

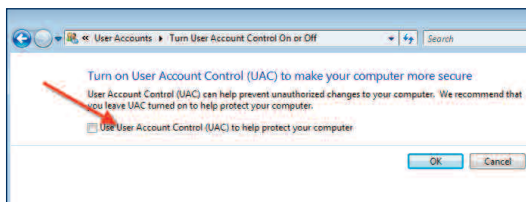
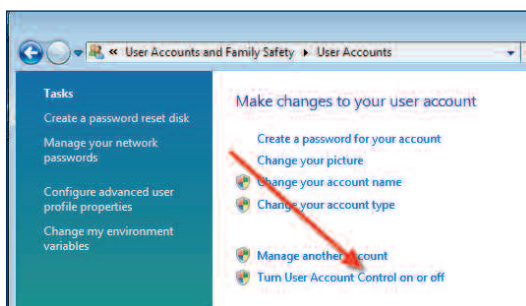
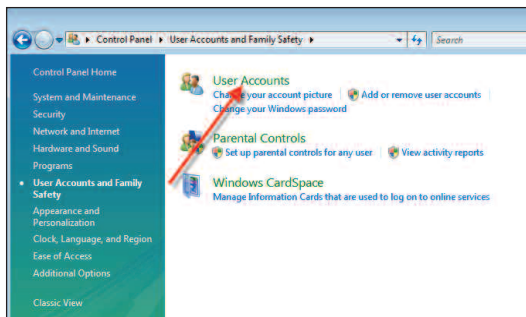


# Step-By-Step Instructions To Save/Back Up Data In Your Current TRUEmanager™ Program To Transfer To New TRUEmanager™ Diabetes Management Software 3.2.1.9


1. If using Microsoft® Windows® Vista®, open the control panel and navigate to **User Account Settings**. Turn off **User Account Settings** by unchecking the check box. If using Microsoft® Windows® XP Professional, skip to Step 2.

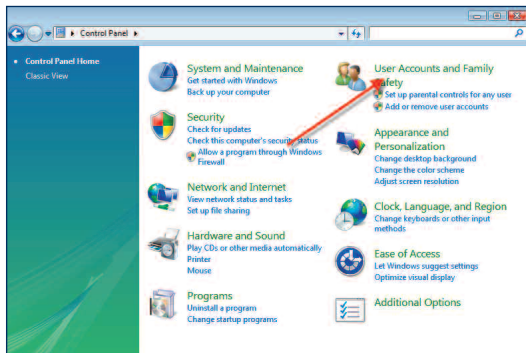

2. Start your current TRUEmanager™ program. From the blood drop menu, click on **Backup Data** option from the menu.

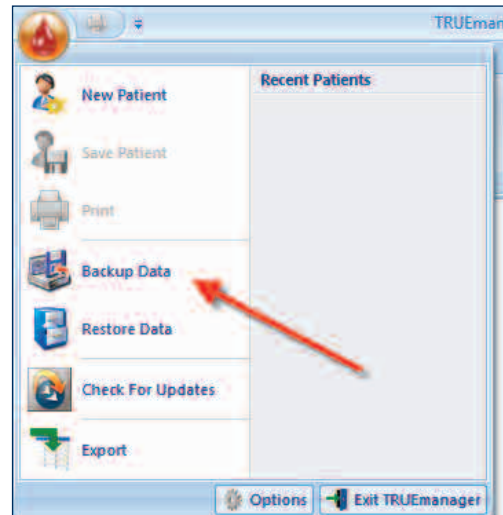


3. When prompted, save your backup file by selecting a safe location where you can easily locate it, in order to restore the backup file to the new TRUEmanager™ program 3.2.1.9 once it is installed.

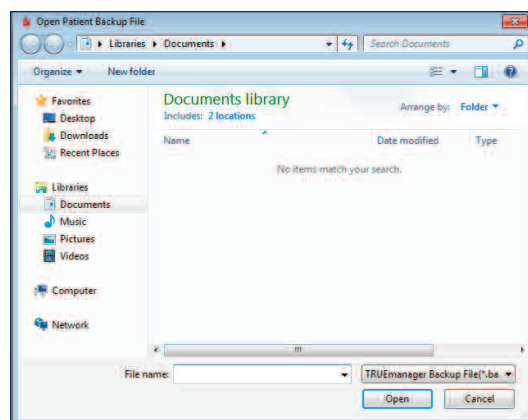


4. After the backup data is complete, close your current TRUEmanager™ program.


5. Click on **“Start”** and open the control panel. Locate the **TRUEmanager™ Diabetes Management Software** from the program list and click on **“Uninstall”**.

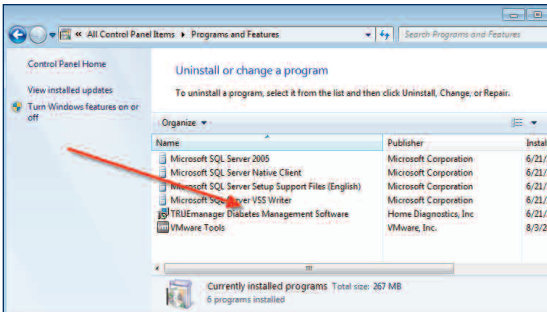


8. Select the **“HDI Database Engine”** from the instance list, and click **“Next”**.

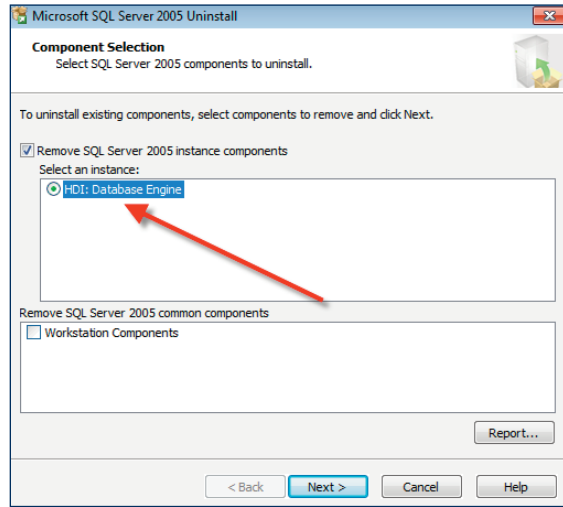


6. Confirm your selection to uninstall your current TRUEmanager™ program by clicking on **“Yes”**.

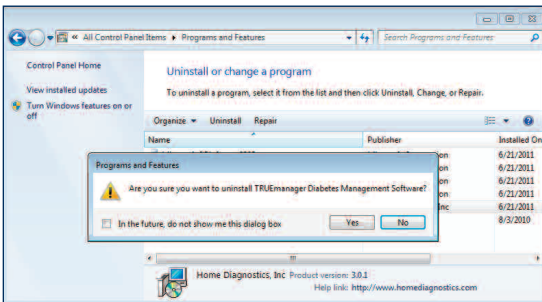

9. On the next screen, click **“Finish”**, and the uninstall of your current TRUEmanager™ program (3.0) will be complete.

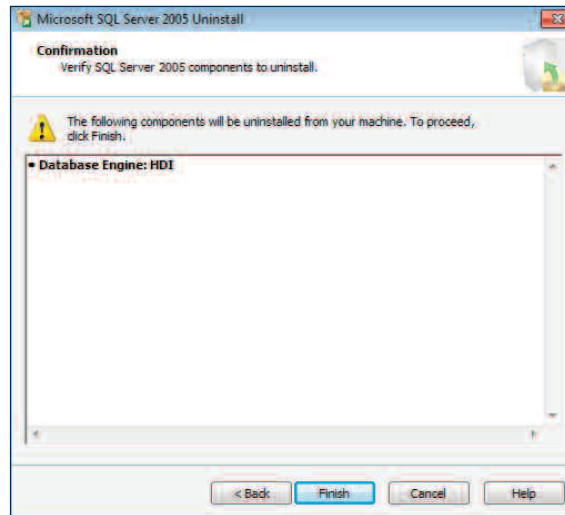


7. Next, you need to uninstall Microsoft® Sequel Server® 2005. Locate **“Microsoft® SQL Server® 2005”** on the control panel screen and select the program, then click **“Uninstall”**. The Microsoft® SQL Server® uninstall screen will appear with a list of SQL Server instances.

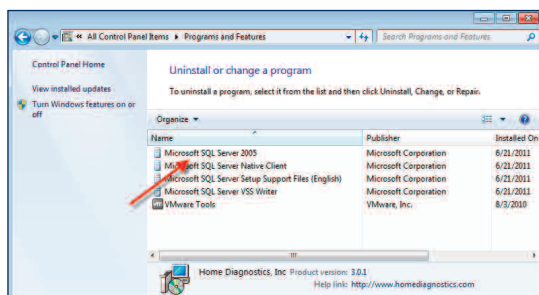

10. You are now ready to begin the installation of the upgraded TRUEmanager™ Diabetes Management Software, version 3.2.1.9. Refer to the owner’s booklet or follow the install wizard for installation of the upgraded software.

11. After TRUEmanager™ version 3.2.1.9 is successfully installed, start the program. Click on the **Blood Drop** on the open screen and select **“Restore Data”**.
  
12. Under the file name, select your backup file that you created in Step 3, and click the **“Open”** button. This will complete the restore of your backup data file into the new TRUEmanager™ program.

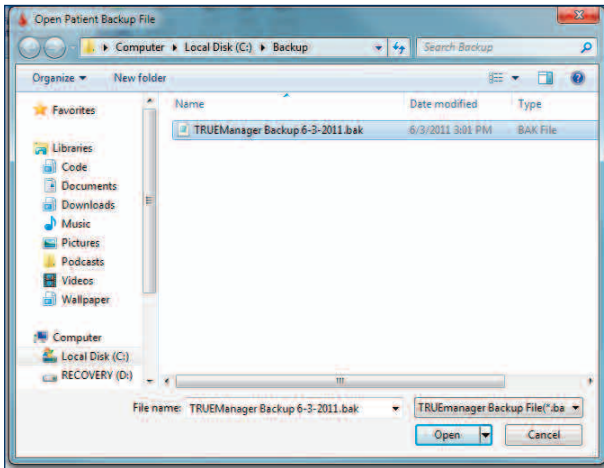

NICO-2373 © 07/11 Nipro Diagnostics, Inc. TRUEmanager, and the Nipro Diagnostics logo are trademarks of Nipro Diagnostics, Inc. All other product names and brand names are trademarks of their respective owners.